

# Comparison of Autorefractors and Retinoscopy with Subjective Corrections in Myopia and Hypermetropia

Dr. Taarika G <sup>1</sup>, Dr N Divya <sup>2</sup>, Dr. Abinaya Ramakrishnan<sup>3\*</sup>

<sup>1</sup> Junior Resident, Department of Ophthalmology , Saveetha Medical College ,Thandalam, Chennai, Tamil Nadu, India

<sup>2</sup> Associate Professor, Department of Ophthalmology , Saveetha Medical College ,Thandalam, Chennai, Tamil Nadu, India

<sup>3</sup> Junior Resident, Department of Ophthalmology , Saveetha Medical College ,Thandalam, Chennai, Tamil Nadu, India

**Abstract: Introduction:** Since Autorefractors nowadays have become mainstream and available in almost all clinical setups Autorefractors to make measurements swiftly. So in such a situation , it is necessary to compare the results of different refraction measurement devices including Autorefractors and retinoscopy with subjective corrections in Myopia and Hypermetropia.

**Methods:** This is a descriptive study done among 100 patients visiting Ophthalmology OPD with Myopia and Hypermetropia in Saveetha medical college selected by convenience Sampling . The data collect ed will be tabulated and analyzed using SPSS.

**Results:** Patients were divided into two age groups to find out age wise distribution of type of refractive errors and comparing the results from the subjective examination and results given by the Autorefractive meter it is clearly from this study that the difference between two methods was almost negligible and that Autorefractors are also a reliable method of measurement in a large clinical setup. But, on the other hand, manual retinoscopy still prove to be far better and efficacious technique yielding accurate results when it is used to check for refractive errors in individuals

**Conclusion:** In this study, we conclude that autorefractors are also reliable and can also be used to estimate refractive errors in a clinical setup, even though manual retinoscopy remains the most accurate and efficacious method..

## 1. INTRODUCTION

Refractive errors are a type of vision problem that makes it hard to see clearly. They happen when the shape of your eye keeps light from focusing correctly on your retina. Refractive errors are the most common type of vision problem. Emmetropia is a condition where in parallel rays of light are focused on the retina when the accommodation is at rest. If the light rays are not focused on the retina but these are focused behind or in front of the retina, the person is unable to see the objects clearly and the condition is called ametropia. When the rays of light are focused behind the retina the condition is called hypermetropia and when the rays are focused in front of the retina the condition is called myopia.

Myopia and hypermetropia are further divided into various types namely axial, curvatural and index depending upon the causative factor involved. The extent to which the refractive system of the eye is faulty in focusing the rays of light on retina is called error of refraction [1].

India is densely populated country, and thus, a faster technique to calculate refractive errors easily, has created a niche in the day-to-day practices of the ophthalmic surgeon. cycloplegic retinoscopy remains the gold standard to assess the refractive error. However, retinoscopy is limited by the time required for the examination and patient discomfort. More recently, autorefractors (ARs) have become widely used to objectively assess refractive status.

Conventional closed-loop ARs use a fogging mechanism to avoid accommodation during measurement. Although evidence suggests that the accuracy and repeatability of noncycloplegic autorefraction are reasonable, other

factors, such as “instrument myopia” which is caused by proximal accommodation, may not be adequately neutralized by fogging techniques. Hence, several studies have recommended measurements under cycloplegic conditions to ensure the accuracy of results [2].

Table-mounted, hand-held, and video retinoscopy autorefractors are three popular automated devices that allow more rapid evaluations of refractive status. Although these instruments can be used either with or without cycloplegia, cycloplegic refraction measurements should be preferred because of strong accommodation in children [3].

The aim of the study was to compare the results of different refraction measurement devices including autorefractor and retinoscopy with subjective corrections in myopia and hypermetropia.

## 2. METHODOLOGY

This descriptive study will be conducted in Saveetha medical college and hospital. Patients visiting Ophthalmology OPD with myopia and hypermetropia who are willing to participate will be included in the study and will be tested for subjective correction in myopia and hypermetropia using autorefractors and retinoscopy.

Sampling: Convenience sampling.

Sample size: 100

The data collected will be tabulated and analyzed using SPSS.

Inclusion criteria: All patients visiting Ophthalmology OPD with myopia and hypermetropia in Saveetha Medical College who are willing to participate.

Exclusion criteria: Patients with other causes of defective vision like corneal opacity, lens changes, retinal problems and glaucoma.

## 3. RESULTS

As the refractive errors of two eyes in all patients were related, so only data from 100 right eyes of patients were analyzed. Patients were divided in two age groups to find out age wise distribution of type of refractive error. In group 1 patients were  $\leq 10$  years and in group 2 patients were  $> 10$  years of age. Out of 100 patients, 37 were in group 1 and 63 were in group 2. In group 1 among 37 patients 17 were myopic and 20 were hypermetropic. In group 2 among 63 patients 20 were myopic and 43 were hypermetropic. p value was  $< 0.005$  which was statistically significant (table 1).


Firstly results of spherical errors given by autorefractometer and subjective method were compared 30 myopic patients had mean and standard deviation of differences  $-0.15 \pm 0.87$  resulted in p value of 0.30 whereas 61 hypermetropic patients had mean and standard deviation of differences  $0.16 \pm 0.14$  resulted in p value of 0.184. When results of spherical errors given by retinoscopy and subjective method were compared 30 myopic patients had mean and standard deviation of differences  $-0.13 \pm 0.62$  resulted in p value of 0.306, whereas 61 hypermetropic patients had mean and standard deviation of differences  $0.176 \pm 0.52$  resulted in p value of 0.276. When results of spherical errors given by autorefractometer and retinoscopy and were compared 30 myopic patients had mean and standard deviation of differences  $-0.03 \pm 0.15$  resulted in p value of 0.277 whereas 61 hypermetropic patients had mean and standard deviation of difference  $-0.02 \pm 0.14$  resulted in p value of 0.011\*.

Secondly results of cylindrical errors given by autorefractometer and subjective method were compared 24 myopic patients had mean and standard deviation of differences  $-0.18 \pm 0.59$  resulted in p value of 0.165 whereas 04 hypermetropic patients

had mean and standard deviation of differences  $-0.39 \pm 0.24$  resulted in p value of 0.373. When results of cylindrical errors given by retinoscopy and subjective method were compared 24 myopic patients had mean and standard deviation of differences  $-0.22 \pm 0.77$  resulted in p value of 0.083 whereas in 04 hypermetropic patient had mean and standard deviation of differences  $0.022 \pm 0.454$  and resulted in p value of 0.696. When results of cylindrical errors given by autorefractometer and retinoscopy and were compared 24 myopic patients had mean and standard deviation of differences  $-0.14 \pm 0.82$  resulted in p value of 0.058 whereas 03 hypermetropic patients had mean and standard deviation of differences  $0.040 \pm 0.46$  resulted in p value of 0.500

Thirdly results of spherical equivalence given by autorefractometer and subjective method were compared 42 myopic patients had mean and standard deviation of differences  $-0.25 \pm 0.80$  resulted in p value of 0.211 whereas 58 hypermetropic patients had mean and standard deviation of differences  $-0.0170 \pm 0.145$  resulted in p value of 0.354. When results of spherical equivalence errors given by retinoscopy and subjective method were compared 42 myopic patients had mean and standard deviation of differences  $-0.12 \pm 0.78$  resulted in p value of 0.320 whereas in 58 hypermetropic patient had mean and standard deviation of differences  $-0.155 \pm 0.57$  resulted in p value of 0.023. When results of spherical equivalence errors given by autorefractometer and retinoscopy were compared 42 myopic patients had mean and standard deviation of difference  $-0.03 \pm 0.16$  resulted in p value of 0.349 whereas 58 hypermetropic patients had mean and standard deviation of difference  $0.23 \pm 0.35$  resulted in p value of 0.373 (table 2)

**Table 2:**

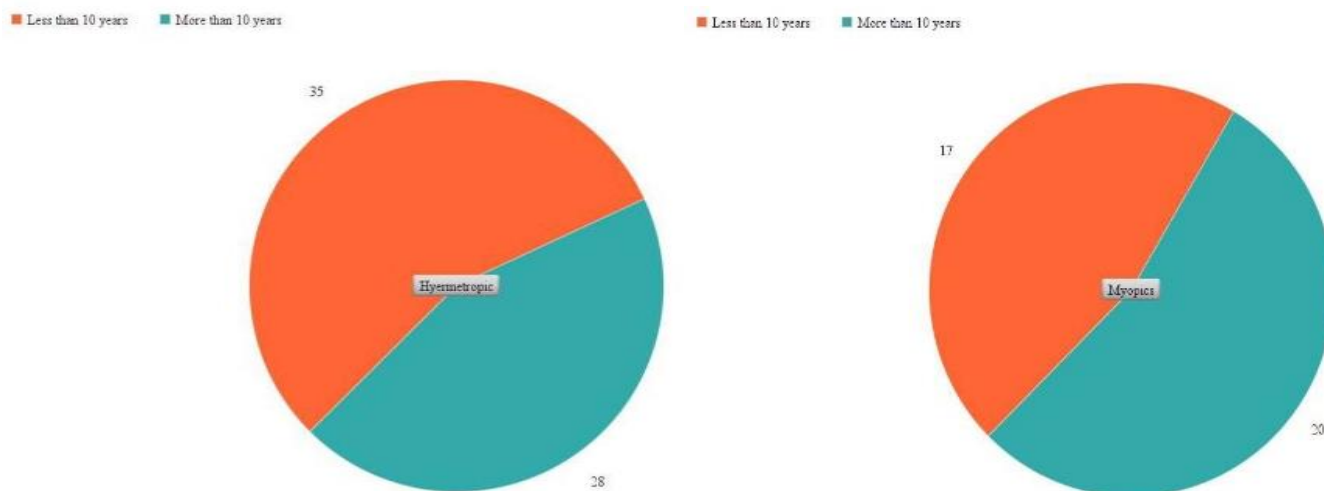

Parameter			Myopic cases			Hypermetropic cases		
			N	MEAN + SD Of Difference	P value	N	MEAN + SD Of Difference	P value
Cycloplegia	Spherical	Autoref Vs Subjective	30	$-0.15 \pm 0.87$	0.329	61	$0.167 \pm 0.144$	0.184
		Retinoscopy Vs Subjective	30	$-0.13 \pm 0.62$	0.306	61	$0.176 \pm 0.52$	0.276
		Autoref Vs Retinoscopy	30	$-0.03 \pm 0.15$	0.277	61	$-0.02 \pm 0.14$	0.011
	Cylindrical	Autoref Vs Subjective	24	$-0.18 \pm 0.59$	0.165	4	$-0.390 \pm 0.24$	0.373
		Retinoscopy Vs Subjective	24	$-0.22 \pm 0.77$	0.083	4	$0.022 \pm 0.454$	0.696
		Autoref Vs Retinoscopy	24	$-0.14 \pm 0.82$	0.058	4	$0.040 \pm 0.463$	0.500
	Spherical Equivalent	Autoref Vs Subjective	42	$-0.25 \pm 0.80$	0.211	58	$-0.017 \pm 0.145$	0.354
		Retinoscopy Vs Subjective	42	$-0.12 \pm 0.78$	0.320	58	$0.155 \pm 0.57$	0.023
		Autoref Vs Retinoscopy	42	$0.03 \pm 0.16$	0.349	58	$-0.23 \pm 0.35$	0.373

#### 4. DISCUSSION

In this study 100 patients with myopia and hypermetropia were tested using retinoscope, autorefractometer and subjective methods after using a cycloplegic. Refractive error is one of the most important preventable causes of blindness and therefore it proves right to use the best instrument for testing it. Therefore, this study was undertaken with the main aim of comparing the efficiency of retinoscopy, autorefractometer and subjective methods over each other. The use of cycloplegic was because to neutralize the excess accommodative effort in individuals wearing glasses with minus over correction as it may lead to myopia. This point is also justified in a study by Hepsen IF et al, wherein it was observed that excess accommodation is one of the factors responsible for increased prevalence of myopia among children<sup>14</sup>.

In this study, there is a closer agreement between results obtained using autorefractometer and other refraction methods regarding the cylindrical component and poorer agreement with regard to the spherical component. These findings are in line with findings of a study by Adyanthaya S et al and others<sup>13, 16</sup>. In an other study conducted by Adyanthaya S et al, although both retinoscopy and autorefractometer had comparable diagnostic accuracy, higher correlation was seen with retinoscopy for spherical error and higher correlation was seen with autorefractometer for cylindrical error and axis deviation<sup>13</sup>. In a study conducted by Jorge J et al, for the sphere power component, retinoscopy and subjective refraction had higher agreement and for cylindrical power and axis autorefractometer and retinoscopy had similar agreement<sup>15</sup>. This is unlike the results found in non cycloplegic conditions like the ones by Mukash SN et al and Hashemi H et al where it was be over minus in myopic and over plus in hyperopic cases<sup>17, 18</sup>. In a study conducted by Verboven L et al, the results obtained through autorefractometers is superior and accurate than those obtained through retinoscopy and that it avoids the examination time required by physicians unlike retinoscopy<sup>8</sup>. Similarly in a study conducted by Choong YF et al, autorefractometer had higher sensitivity and specificity for myopia and hypermetropia<sup>2</sup>. In a study conducted by Hashemi H et al autorefraction gave plus results overall<sup>18</sup> and in a study conducted by Prabhakaran et al autorefraction gave minus results overall. The discrepancies in the results must be due to the difference in sample size and demographic composition of the study population.

In our study, the refractive status of school age children was assessed using conventional retinoscopy and autorefraction, and the accuracy of these objective methods was compared against subjective refraction. Both retinoscopy and autorefraction were found to have comparable diagnostic accuracy. However, it was observed that higher correlation was found with retinoscopy for spherical error, while autorefraction correlated better with subjective correction for cylindrical error and axis estimation. In our study, the refractive status of school age children was assessed using conventional retinoscopy and autorefraction, and the accuracy of these objective methods was compared against subjective refraction.

Both retinoscopy and autorefraction were found to have comparable diagnostic accuracy. However, it was observed that higher correlation was found with retinoscopy for spherical error, while autorefraction correlated better with subjective correction for cylindrical error and axis estimation. In this study we thus conclude that although autorefractometers have good efficacy and is highly useful for testing refractive errors in a large clinical setup, manual retinoscopy is far better and efficacious technique yielding accurate results when used to check for refractive errors in individuals. This finding is also observed in several other similar studies done across the globe. In the study carried out by Adyanthaya S et al, they have concluded that conventional retinoscopy is still the most accurate method for estimating refractive status and can be considered as a very good starting point for subjective refraction<sup>13</sup>.

#### 5. CONCLUSION

In this study we thus conclude that although autorefractometers have good efficacy and is highly useful for testing refractive errors in a large clinical setup, manual retinoscopy is far better and efficacious technique yielding accurate results when used to check for refractive errors in individuals

#### 6. REFERENCES

- [1] Prabhakar SK. Study on accommodation by autorefraction and dynamic refraction in children. *J Optom.* 2014;7:193– 202.

- [2] Choong YF, Chen AH, Goh PP. A Comparison of Autorefractometry and Subjective Refraction With and Without Cycloplegia in Primary School Children. *Am J Ophthalmol*. 2006;142:68–74.
- [3] Rotsos T, Grigoriou D, Kokkolaki A, Manios N. A comparison of manifest refractions, cycloplegic refractions and retinoscopy on the RMA-3000 autorefractometer in children aged 3 to 15 years. *Clin Ophthalmol*. 2009;3: 429–431.
- [4] Uras R, Belfort R, Hofling-Lima AL, Martins EL. Ganger, et al. Autorefractometer, Retinoscope and Subjective Method International Journal of Contemporary Medical Research ISSN (Online): 2393-915X; (Print): 2454-7379 | ICV (2015): 77.83 | Volume 4 | Issue 3 | March 2017 743 Automatic objective refraction and clinical refraction - a comparative analysis *Arq Bras Oftalmol*. 2001;64:33-8.
- [5] Bullimore MA, Fusaro RE, Adams CW. The repeatability of automated and clinician refraction. *Optom Vis Sci*. 1998;75:617-22.
- [6] Tongue AC. Refractive error in children. *Pediatr Clin North Am*. 1987;34:1426-1437.
- [7] Rosenfield M, Chin NN. Repeatability of subjective and objective refraction. *Ophthalmol Vis Sci*. 1995;72:577-579.
- [8] Verboven L, Missoten L, Possibilities and limitations of refraction measurement by an automatic refractor. *Bull Sec Belge Ophthal*. 1982;201:65-70.
- [9] Williams C, Lumb R, Harvey I, Sparrow JM. Screening for refractive errors with the Topcon PR2000 Pediatric Refractometer. *Invest Ophthalmol Vis Sci*. 2000;41:1031- 7.
- [10] Isenberg SJ, Del Signore M, Madani-Becker G. Use of the HARK autorefractor in children *Am J Ophthalmol*. 2001;131:438-41.
- [11] Abraham Ipe, Priyanka Shibu, Rohith Skariah. Prevalence of refractive errors and the extent of correction possible with conservative methods, among patients visiting a tertiary care hospital in South Kerala. *International Journal of Contemporary Medical Research*. 2016;3:2754-2756.
- [12] Puspendu Das, Ruma Das, Praveer Kumar Shrivastava, Abhisek Mondal. A clinical study on the correlation between axial length, intraocular pressure and central corneal thickness in myopic eyes. *International Journal of Contemporary Medical Research*. 2016;3:1141-1144.
- [13] Adyanthaya S , Abhilash B, A comparison between retinoscopy and autorefractometry in acceptance of subjective correction in school age children. *Indian J Clin Exp Ophthalmol* 2020;6(3):418-421
- [14] Hepsen IF, Evereklioglu C, Bayramlar H. The effect of reading and near-work on the development of myopia in emmetropic boys: a prospective, controlled, three-year follow-up study. *Vision research*. 2001 Sep 1;41(19):2511-20.
- [15] Jorge J, Queiros A, Almeida JB, Parafita MA. Retinoscopy/autorefractometry: which is the best starting point for a noncycloplegic refraction?. *Optometry and vision science*. 2005 Jan 1;82(1):64-8.
- [16] D A Goss T Grosvenor Reliability of refraction--a literature review *J Am Optom Assoc* 1996;67(10):1930
- [17] Mukash SN, Kayembe DL, Mwanza JC. Agreement Between Retinoscopy, Autorefractometry and Subjective Refraction for Determining Refractive Errors in Congolese Children. *Clinical Optometry*. 2021;13:129.
- [18] Hashemi H, Khabazkhoob M, Asharlous A, Yekta A, Emamian MH, Fotouhi A. Overestimation of hyperopia with autorefractometry compared with retinoscopy under cycloplegia in school-age children. *British Journal of Ophthalmology*. 2018 Dec 1;102(12):1717-22.

DOI: <https://doi.org/10.15379/ijmst.v10i1.2682>

This is an open access article licensed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0/>), which permits unrestricted, non-commercial use, distribution and reproduction in any medium, provided the work is properly cited.